



**University of
Zurich^{UZH}**

**Zurich Open Repository and
Archive**

University of Zurich
University Library
Strickhofstrasse 39
CH-8057 Zurich
www.zora.uzh.ch

Year: 2014

Static biofilm removal around ultrasonic tips in vitro

Thurnheer, Thomas ; Rohrer, Elodie ; Belibasakis, Georgios N ; Attin, Thomas ; Schmidlin, Patrick R

Abstract: **OBJECTIVES:** This study aims to investigate the biofilm removal capacity of two ultrasonic tips under standardized conditions using a multi-species biofilm model. **METHODS:** Six-species biofilms were grown on hydroxyapatite discs for 64.5 h and were treated for 15 s with a standardized load of 40 g with a piezoelectric or magnetostrictive device. Tips were applied either with the tip end or with the side facing downwards. Detached bacteria were determined in the supernatant and colony-forming units (CFUs) counted after 72 h of incubation. Untreated specimens served as controls. Moreover, the biofilms remaining on the hydroxyapatite surface after treatment were stained using the Live/Dead stain, and the pattern of their detachment was assessed by confocal laser scanning microscopy (CLSM). **RESULTS:** As compared to the untreated control, it was found that only a side application of the magnetostrictive device was able to remove efficiently the biofilm. In contrast, its tip application as well as both applications of the piezoelectric device removed significantly less bacteria from the biofilm structure. These findings were corroborated by CLSM observation. **CONCLUSION:** Both ultrasonic tips under investigations led to bacterial detachment, but the action mode as well as the tip configuration and adaptation appeared to be influenced by the biofilm removal effectiveness. **CLINICAL RELEVANCE:** Biofilm removal remains a main goal of ultrasonic debridement. This should be reflected in respective laboratory investigations. The presented combination of methods applied on a multi-species biofilm model in vitro allows the evaluation of the effectiveness of different ultrasonic scaler applications.

DOI: <https://doi.org/10.1007/s00784-013-1157-2>

Posted at the Zurich Open Repository and Archive, University of Zurich

ZORA URL: <https://doi.org/10.5167/uzh-87186>

Journal Article

Accepted Version

Originally published at:

Thurnheer, Thomas; Rohrer, Elodie; Belibasakis, Georgios N; Attin, Thomas; Schmidlin, Patrick R (2014). Static biofilm removal around ultrasonic tips in vitro. *Clinical Oral Investigations*, 18(7):1779-1784.

DOI: <https://doi.org/10.1007/s00784-013-1157-2>

Static biofilm removal around ultrasonic tips in vitro

Thurnheer Thomas, Dr. sc. nat. ETH¹, Rohrer Elodie, med. dent. pract.²; Georgios N. Belibasakis, PD PhD.³, Thomas Attin, Prof. Dr. med. dent.⁴, Patrick R. Schmidlin, Prof. Dr. med. dent.⁵

¹ Scientist, Institute of Oral Biology, Section for Oral Microbiology and General Immunology, Center of Dental Medicine, University of Zurich, Switzerland

² Doctoral student, Clinic of Preventive Dentistry, Periodontology and Cariology, Center of Dental Medicine, University of Zurich, Switzerland

³ Interim Head, Section for Oral Microbiology and General Immunology, Institute of Oral Biology, Center of Dental Medicine, University of Zurich, Switzerland

⁴ Director and Head, Clinic of Preventive Dentistry, Periodontology and Cariology, Center of Dental Medicine, University of Zurich, Switzerland

⁵ Head Division of Periodontology, Clinic of Preventive Dentistry, Periodontology and Cariology, Center of Dental Medicine, University of Zurich, Switzerland

Corresponding author:

Prof. Dr. med. dent. Patrick R. Schmidlin

Clinic of Preventive Dentistry, Periodontology and Cariology, Center of Dental Medicine, University of Zurich, Switzerland, Plattenstrasse 11, CH 8032 Zürich, Switzerland; e-mail: patrick.schmidlin@zzm.uzh.ch; telephone: +41 44 634 32 84; fax: +41 44 634 43 08.

Static biofilm removal around ultrasonic tips in vitro

Abstract

Objectives: To investigate the biofilm removal capacity of two ultrasonic tips under standardized conditions using a multi-species biofilm model.

Methods: Six-species biofilms were grown on hydroxyapatite discs for 64.5 h and were treated for 15 s with a standardized load of 40 g with a piezoelectric or magnetostrictive device. Tips were applied either with the tip end or with the side facing downwards. Detached bacteria were determined in the supernatant and colony-forming units (CFU) counted after 72 h incubation. Untreated specimens served as controls. Moreover, the biofilms remaining on the hydroxyapatite surface after treatment were stained using the Live/Dead stain and the pattern of their detachment was assessed by confocal laser scanning microscopy (CLSM).

Results: As compared to the untreated control, it was found that only a side application of the magnetostrictive device was able to remove efficiently the biofilm. In contrast, its tip application, as was well as both applications of the piezoelectric device removed significantly less bacteria from the biofilm structure. These findings were corroborated by CLSM observation.

Conclusion: Both ultrasonic tips under investigations led to bacterial detachment, but the action mode as well as the tip configuration and adaptation appeared influenced the biofilm removal effectiveness..

Clinical relevance: Biofilm removal remains a main goal of ultrasonic debridement. This should be reflected in respective laboratory investigations. The presented combination of methods applied on a multispecies biofilm model in vitro allows the distinction between the effectiveness of different ultrasonic scaler applications.

Key words: Biofilm, Periodontitis, Ultrasonic scaler, Vibration, Tooth cleaning

Introduction

The current approach to treat periodontitis is primarily focusing on the elimination of bacterial biofilms, which is still considered the primary etiologic factor of soft tissue inflammation [1]. Besides the traditional treatment using hand curettes, ultrasonic devices have become a well-documented and effective treatment modality [2]. The removal of plaque from tooth surfaces with ultrasound is achieved primarily by a vibratory machining action of the instrument tip [3]. The latter is supported by cavitation activity [4] and acoustic microstreaming in water or within the associated cooling water supply [4, 5]. The physical action is thereby related to the displacement amplitude of the instrument tip and an elliptical motion, which was demonstrated for both, piezoelectric and magnetostrictive ultrasonic devices [6-9]. Various factors influencing these movements have been identified, for example loading, generator power or the amount of cooling water [4, 8, 9]. But also the design and the length of the probe influence the amount of cavitation activity generated but again, the application of load affects the production of cavitation at the most clinically relevant area - the tip [10].

Whereas the mechanical action of ultrasonic devices has been widely investigated under different laboratory settings, there is still a need to assess these effects on a laboratory surrogate model, which provides insights in the resulting biofilm removal efficiency [11]. Therefore, we aimed to assess differences in hydrodynamic action in terms of biofilm removal and a fluorescence *in situ* hybridisation/confocal laser scanning microscopy (FISH/CLSM) analysis in an *in vitro* multi-species biofilm model. In this context, the well-established and validated “Zürich” biofilm model was selected, which consisted of six species [12]. This allowed for the formation of reproducible biofilms and treatment under standardized conditions *in vitro*.

A magnetostrictive and a piezoelectric ultrasound device with different action mode and tip designs were investigated. A positive control treatment consisting of manual scraping using a plastic curette allowed for the determination of the complete biofilm mass. Therefore, as primary outcome, we hypothesized that an effective static ultrasonic action using a test devices would result in comparable total CFU values when compared to the positive control, whereas any less effective treatment would leave more biofilms behind attached on the hydroxyapatite (HA) discs and lead to decreased total CFU values. In addition, we hypothesized that a slim tip design of a magnetostrictive device would lead to greater biofilm removal as compared to a more rigid piezoelectric tip. These differences may become evident not only in terms of quantitative removal of viable bacteria with the proposed method, but also regarding a visual examination.

Material and Methods

Biofilm Preparation

In this study, a modified multi-species biofilm model was used [13] in order to mimic more accurately the fast and feast periods experienced by natural dental plaque, rendering the biofilm more sticky and adherent. In brief, *Actinomyces oris* (formerly *Actinomyces naeshundii*) OMZ 745, *Veillonella dispar* OMZ 493, *Fusobacterium nucleatum* OMZ 598, *Streptococcus mutans* OMZ 918, *Streptococcus oralis* OMZ 607 and *Candida albicans* OMZ 110 were used to grow biofilms in 24-well polystyrene cell culture plates on HA discs (Ø 9 mm; Clarkson Chromatography Products, South Williamsport, PA, USA) that had been preconditioned (pellicle-coated) in 1 ml processed whole unstimulated pooled saliva and incubated for 4 hours at room temperature. To start a biofilm experiment, discs were covered with 1 ml of growth medium (saliva/mFUM) and 200 µl of a microbial suspension prepared from equal volumes and densities of each strain. mFUM corresponds to a well-established tryptone-yeast-based broth medium designated as FUM [14] and modified by supplementing 67 mM Sørensen's buffer (final pH 7.2). The carbohydrate concentration in mFUM was 0.3% (w/v), and consisted of glucose for the first 16.5 h and from then on of a 1:1 (w/w) mixture of glucose and sucrose (see below). Biofilms were incubated anaerobically at 37 °C for 64.5 h. After inoculation the discs remained for 45 min in the feeding solution containing 0.3% glucose. Afterwards, they were subjected to three consecutive 1 min dip-washes in 2 ml 0.9% NaCl to remove growth medium and free floating cells but not microorganisms adhering firmly to the HA discs. The biofilms were then further incubated in new wells containing 1 ml of saliva only. After 16.5, 20.5, 24.5, 40.5, 44.5 and 48.5 h biofilms were pulse-fed by transferring the discs for 45 min into 30% saliva / 70% mFUM with 0.15% glucose and 0.15% sucrose. They were washed again as described above and re-incubated in saliva. Fresh saliva was provided after 16.5 h and 40.5 h. After 64.5 h the biofilms were dip-washed again prior to processing for further treatments and analyses (see below).

Treatments

Biofilms were treated with two different ultrasonic scalers, namely a piezoelectric miniMaster generator (EMS, Nyon, Switzerland) and a Cavitron Select SPS generator (Dentsply, York, PA, USA) at medium power. The insert designs used with these generators included the P-tip (with the EMS generator) and the straight Slimline insert (with the Dentsply generator; Fig. 1).

Prior to treatment, the HA discs were fixed in teflon molds and put in wells of a 96-well cell culture plate that was placed on a balance in order to apply defined pressure during the treatment (Fig. 1). Treatments were randomly allocated and four discs were used for each intervention: Four samples were treated for 15 s at a pressure of 40 g with the tip of the piezoelectric scaler, while another four biofilms were treated under the same conditions, but using the convex front part of the same scaler (referred as the "side" throughout the manuscript; Fig. 1). The same procedures were performed for the magnetostrictive scaler. Standardized application force for each treatment method was achieved by mounting the teeth in a specially adapted pressure sensitive electronic device (TM 503 Power Module, Tektronix®, Inc., Beaverton, Oregon, USA). After every treatment, the biofilms were rinsed with 1.6 ml sterile saline. Four control discs were left untreated except for rinsing. Biofilms of these samples were scraped off manually (control) in order to determine the total CFU of firmly adhering bacteria.

While three of the four discs were used for the analysis of the biofilm mass, one randomly selected fourth sample was used for CLSM analysis, as described below. Therefore, the experiments to assess the biofilm removal were carried out in triplicates, resulting in N=9 samples in total per group.

Analysis of Biofilm removal

To measure the amount of potentially growing bacteria without ultrasonic treatment, biofilms were manually scraped-off (Perio SoftScaler, Kerr, Bioggio, Switzerland) the discs and the latter were rinsed with 1.6 ml sterile saline to remove non-adherent bacteria.

After treatment the supernatant was collected (1.6. ml) and serial dilutions of suspended biofilm bacteria were prepared in 0.9% NaCl and 50 µl aliquots were plated on Columbia blood agar supplemented with 5% whole human blood to estimate total CFU and agar plates were incubated anaerobically at 37 °C for 72 h. Data were scored as total CFU per biofilm.

All microbiological tests and analyses were performed strictly blinded to the nature of the previous treatment of the individual discs.

Staining of biofilms and CLSM

For CLSM treated as well as untreated biofilms were stained using the LIVE/DEAD BacLight bacterial viability assay (Invitrogen, Zug, Switzerland) according to the instructions of the manufacturer. After 20 min staining excess dye was gently aspirated from the discs without

touching the biofilms. They were embedded upside-down in 20 μ l of Mowiol [15], and stored at room temperature in the dark for at least 6 h prior to microscopic examination.

Stained biofilms were examined by CLSM at randomly selected positions using a Leica TCS SP5 (Leica Microsystems, Heidelberg GmbH, Germany) with a x20/0.8 numerical aperture (NA) and x63/1.4 NA oil immersion objective lens in conjunction with 488-nm laser excitation and 530-nm emission filters for Syto 9 (live stain), and 561-nm laser excitation and 640-nm emission filters for propidium iodide (dead stain). Image acquisition was done in 8-line average mode and the data were processed using Imaris 7.2.2 (Bitplane AG, Zurich, Switzerland).

Statistical Analysis

Descriptive statistics of the data were performed with SPSS (version 20.0) and illustrated with box plots. The \log_{10} -transformed data met the requirements for parametric analysis. Hence differences between treatments were analyzed by a one-way analysis of variance (ANOVA) followed by the Scheffe-post-hoc tests (significance level $p < 0.05$).

Results

The effect of the different instrumentation procedures on the HA-grown biofilms was evaluated by means of defining the bacterial CFUs in the culture supernatants, following the treatments (Fig. 2). As compared to the untreated control, which displayed the maximum bacterial mass to be potentially dislodged, it was found that only a side application of the magnetostrictive device was able to remove a comparable amount of the biofilm. In contrast, its tip application, as well as both applications of the piezoelectric device removed significantly less bacteria.

In figure 3, a representative series of confocal images before and after treatment is presented. The broad image represents a section of the biofilm taken at 5 μ m distance from the surface of the disc and the smaller image shows the corresponding cross-section of the biofilm. The figure confirms the results of the CFU analyses and the Live/Dead staining demonstrates that ultrasonic scaling has no effect on the vitality of the biofilms except for the treatment with the magnetostrictive side application (Fig. 3F). Figure 3A shows the untreated biofilm. The HA disc was confluentlly colonized by a biofilm with a mean thickness of 38 μ m. In figure 3B the biofilm after manual scaling is shown and the image confirms that the whole biofilm was eliminated. Figures 3C and D show the effect of the piezoelectric scaler: Treatment using the

tip removed the biofilm only in the center of the disc (Fig. 3C) whereas a sideways application was somewhat more efficient. In figures 3E and F the treatment of the magnetostrictive device is demonstrated: Apparently, this scaler was able to eliminate more of the *in vitro* biofilm than piezoelectric application mode.

Discussion

This study assessed the direct impact of ultrasonic scaler tips on biofilm removal. This was performed by both conventional culture techniques to determine the removed bacteria in the supernatant, and by visualization using a combination of FISH and CLSM. In general, there is still a great need to assess and standardize biofilm removal procedures for testing the (pre-)cleaning efficiency [16], and there is still limited data available concerning the biofilm removal capacity using different protocols, devices and/or chemicals.

The main finding of this study is that only a side application of the magnetostrictive device was able to remove a considerable amount of the biofilm from the HA surface, as compared to the manually treated control, which displayed the maximum bacterial mass to be potentially dislodged. A tip application, in either the magnetostrictive or the piezoelectric device – in contrast - removed a significantly smaller amount of the biofilm, as evaluated by both CFU counting and CLSM visualization.

The *in vitro* biofilm used in this study is a well-established and validated biofilm model of standardized conditions, consisting of either five or six species representative for supragingival plaque [17, 18]. This model has been proven to provide repeatable results on different materials and has been successfully used to evaluate the antimicrobial potential *in vitro* [12, 19-21]. Although this method still represents a simplified laboratory plaque model, it mimics the complex *in vivo* situation more precisely than a mono-species biofilm and due to a feeding model, the biofilm exerts a sticky consistency, which is comparable to the natural conditions. Hence, this is a suitable experimental model to test the efficiency of ultrasonic scalers in removing supragingival plaque, under standardized conditions.

Regarding the biofilm removal capacity, a previously published study showed comparable numbers of cultivatable bacteria on untreated samples, by investigating colonization and measuring total CFUs [11], which elucidates again the reproducibility of this model with regard to biofilm growth. In addition, the effectiveness of biofilm removal has proven to be largely dependent on the methods applied so far. The treatment with ozone and photodynamic therapy (PDT), for instance, showed only minute effects on the remaining biofilm [19]; the

observed reduction of viable counts by both treatment options was less than one \log_{10} step. In another study, where the efficiency of shock waves was investigated, they effectively removed biofilms by three log steps [11]. In the present study, both the biofilm structure remaining on the HA surface, and the number of detached bacteria were evaluated, following the two treatment modalities. However, since only viable counts were determined, one can drive conclusions only on the viability after treatment, not on bacterial detachment *per se*. That is because non-viable bacteria could also be detached from the HA surface following treatment. This cannot be taken under consideration when measuring the CFUs. Hence, further usage of FISH and CLSM to identify the biofilm remaining on the surface is a suitable complementary approach in the present study.

Relevant work also exists on the mechanisms of non-contact biofilm removal by sonic and other powered toothbrushes, which elucidates the importance of this kind of evaluations to study the efficiency of bacteria removal by physico-mechanical means. A study by Busscher and co-workers showed that sonic brushing at contact removed 92% to 94% of the coadhering and non-coadhering pair under investigation, respectively, but removal decreased with increasing distance between the brush and the pellicle surfaces [22]. Especially non-contact biofilm removal must be regarded as an interplay of hydrodynamic energy transfer through the fluid [23]. The extent to which specific different hydrodynamic factors contribute is still dependent on the specifics of the instruments. On the other hand, He and co-workers found that powered brushing in non-contact mode changed the viscoelastic properties of the oral biofilm resulting in increased penetration of antimicrobial compounds into the biofilm [24,25]. Therefore, even if biofilms are not totally removed by sonic brushing, they may be more susceptible to antimicrobials thereafter.

Walmsley and coworkers mapped the occurrence of cavitation around scaler tips under loaded conditions [10]. The vibration displacement amplitude of ultrasonic scalers increased with the occurrence of cavitation, but factors such as the length of the probe influence the amount of cavitation activity generated. In general, the application of load affects the production of cavitation at the most clinically relevant area, which is the tip of the device.

A standardized load of 40 g was applied in this study. It has been shown that magnetostrictive probes oscillated with greater displacement amplitudes than piezoelectric probes, but still produced similar defects. This may be due to the cross-sectional shape of the probes [8]. In the present study, the same devices and tips were used and these earlier findings could be reproduced in this biofilm model as well. However, the applied loads were higher in the latter case, ranging from 100 g to 200 g. Future studies could use the presented biofilm model to

study the contact free effectiveness of ultrasonic instrumentation using different action modes, power settings and geometries. However, one should keep in mind that the sample arrangement, i.e. the embedding or attachment of the samples may influence the vibration transduction and thus the efficacy of the treatment. The disc material can as well play a role. With this respect it can also be speculated that a slimmer tip may cut into the disc throwing up micron sized particles, which may then add to a slurry increasing cavitation. In the present study, we used an artificial HA disc with a Knoop hardness number of 310, which is in the range of enamel, and no surface damage could be observed. However, this does not exclude the possibility of microscopic damage and it would be of interest to assess this aspect on dentin or other biological surfaces and biomaterials in terms of biofilm removal in combination with surface damage in future studies.

In summary, studies of ultrasonic devices provide valid documentation of their efficiency particularly when using biofilm models and this study provided first insights in the microbiological aspects of working action of ultrasonic scalers under standardized conditions.

Conclusions

Regarding the research hypothesis it was found that both ultrasonic tips under investigations led to bacterial detachment, but the action mode as well as the tip configuration and adaptation appeared influenced the biofilm removal effectiveness.

Acknowledgments

The authors would like to thank Andy Meier and Ruth Graf for their great support in the laboratory. We thank the Centre of Microscopy and Image Analysis (ZMB) of the University of Zurich for their support with confocal microscopy.

Conflict of interest

The authors have no conflicts of interest.

References

1. Badersten A, Nilveus R, Egelberg J (1981) Effect of nonsurgical periodontal therapy. I. Moderately advanced periodontitis. *J Clin Periodontol* 8: 57-72
2. Walmsley AD, Lea SC, Landini G, Moses AJ (2008) Advances in power driven pocket/root instrumentation. *J Clin Periodontol* 35: 22-28
3. Lampe Bless K, Sener B, Dual J, Attin T, Schmidlin PR (2011) Cleaning ability and induced dentin loss of a magnetostrictive ultrasonic instrument at different power settings. *Clin Oral Investig* 15: 241-248
4. Lea SC, Landini G, Walmsley AD (2006) The effect of wear on ultrasonic scaler tip displacement amplitude. *J Clin Periodontol* 33: 37-41
5. Walmsley AD, Laird WR, Williams AR (1984) A model system to demonstrate the role of cavitation activity in ultrasonic scaling. *J Dent Res* 63: 1162-1165
6. Walmsley AD, Laird WR, Williams AR (1986) Displacement amplitude as a measure of the acoustic output of ultrasonic scalers. *Dent Mater* 2: 97-100
7. Walmsley AD, Laird WR, Williams AR (1986) Inherent variability of the performance of the ultrasonic scaler. *J Dent* 14: 121-125
8. Lea SC, Landini G, Walmsley AD (2002) Vibration characteristics of ultrasonic scalers assessed with scanning laser vibrometry. *J Dent* 30: 147-151
9. Lea SC, Felver B, Landini G, Walmsley AD (2009) Three-dimensional analyses of ultrasonic scaler oscillations. *J Clin Periodontol* 36: 44-50
10. Walmsley AD, Lea SC, Felver B, King DC, Price GJ (2013) Mapping cavitation activity around dental ultrasonic tips. *Clin Oral Investig* 17: 1227-34
11. Muller P, Guggenheim B, Attin T, Marlinghaus E, Schmidlin PR (2011) Potential of shock waves to remove calculus and biofilm. *Clin Oral Investig* 15: 959-965
12. Shapiro S, Giertsen E, Guggenheim B (2002) An in vitro oral biofilm model for comparing the efficacy of antimicrobial mouthrinses. *Caries Res* 36: 93-100.
13. Thurnheer T, van der Ploeg JR, Giertsen E, Guggenheim B (2006) Effects of *Streptococcus mutans* gtfC deficiency on mixed oral biofilms in vitro. *Caries Res* 40: 163-171
14. Gmur R, Guggenheim B (1983) Antigenic heterogeneity of *Bacteroides intermedius* as recognized by monoclonal antibodies. *Infect Immun* 42: 459-470

15. Thurnheer T, Gmur R, Shapiro S, Guggenheim B (2003) Mass transport of macromolecules within an in vitro model of supragingival plaque. *Appl Environ Microbiol* 69: 1702-1709
16. Oulahal N, Martial-Gros A, Bonneau M, Blum LJ (2004) Combined effect of chelating agents and ultrasound on biofilm removal from stainless steel surfaces. Application to "Escherichia coli milk" and "Staphylococcus aureus milk" biofilms. *Biofilm* 1: 65-73.
17. Guggenheim B, Giertsen E, Schupbach P, Shapiro S (2001) Validation of an in vitro biofilm model of supragingival plaque. *J Dent Res* 80: 363-370
18. Guggenheim B, Guggenheim M, Gmur R, Giertsen E, Thurnheer T (2004) Application of the Zurich biofilm model to problems of cariology. *Caries Res* 38: 212-222
19. Muller P, Guggenheim B, Schmidlin PR (2007) Efficacy of gasiform ozone and photodynamic therapy on a multispecies oral biofilm in vitro. *Eur J Oral Sci* 115: 77-80.
20. Dezelic T, Guggenheim B and Schmidlin PR. Multi-species biofilm formation on dental materials and an adhesive patch. *Oral Health Prev Dent*, 2009; 7: 47-53.
21. Hofer D, Meier A, Sener B, Guggenheim B, Attin T, Schmidlin PR (2011) Biofilm reduction and staining potential of a 0.05% chlorhexidine rinse containing essential oils. *Int J Dent Hyg* 9: 60-67
22. Busscher HJ, Rustema-Abbing M, Bruinsma, GM, de Jager M, Gottenbos B, van der Mei HC (2003) Non-contact removal of coadhering and non-coadhering bacterial pairs from pellicle surfaces by sonic brushing and de novo adhesion. *Eur J Oral Sci* 111: 459-64
23. Busscher HJ, Jager D, Finger G, Schaefer N, van der Mei HC (2010) Energy transfer, volumetric expansion, and removal of oral biofilms by non-contact brushing. *Eur J Oral Sci* 118: 177-82
24. He Y, Peterson BW, Ren Y, van der Mei HC, Busscher HJ (2013) Antimicrobial penetration in a dual-species oral biofilm after noncontact brushing: an in vitro study. *Clin Oral Invest* 2013 Sep 10. [Epub ahead of print]
25. He Y, Peterson BW, Jongsma MA, Ren Y, Sharma PK, Busscher HJ, van der Mei HC (2013) Stress relaxation analysis facilitates a quantitative approach towards antimicrobial penetration into biofilms. *PLoS One* 27;8:e63750.

FIGURE LEGENDS

Figure 1: Tip design (A/B) and study set-up (C): The different insert designs used in this study as seen from above (left) and sideways (A: P tip; B: Slimline). First, HA discs with established biofilms (a) were put into sterile customized teflon molds (b), which were placed in 96-well plates, and were treated with either a magnetostrictive or piezoelectric ultrasonic device as described in the Materials and Methods section. All tests were carried out in triplicates in three different experiments resulting in a total sample size of N=9 per group.

Figure 2: Box plots of the total CFUs of the untreated control specimens (scrapped-off the HA surface) and the total CFUs release into the supernatant after treatment of biofilms with the different devices. Identical capitals represent results, which do not statistically significantly differ from each other (ANOVA, Scheffe).

Figure 3: CLSM images of in vitro biofilms on the HA surface before and after treatment. Images have been taken along the diameter of the discs and represent only a detail of the whole disc whereat the broad and small strips represent transverse (xy) sections taken at 5 μm above the HA surface and the corresponding cross sections (xz), respectively, with the surface of the biofilm facing downwards. The biofilms were stained using the Live/Dead Viability Kit; live cells appear green, dead cells red. Black areas on the HA surface resulted from complete removal of the biofilm. A: untreated biofilm; B: after manual collection of biofilms; C: piezoelectric scaler tip; D: piezoelectric scaler side; E: magnetorestrictive scaler tip; F: magnetorestrictive scaler side. Scale bar: 500 μm .

Figures

Fig. 1

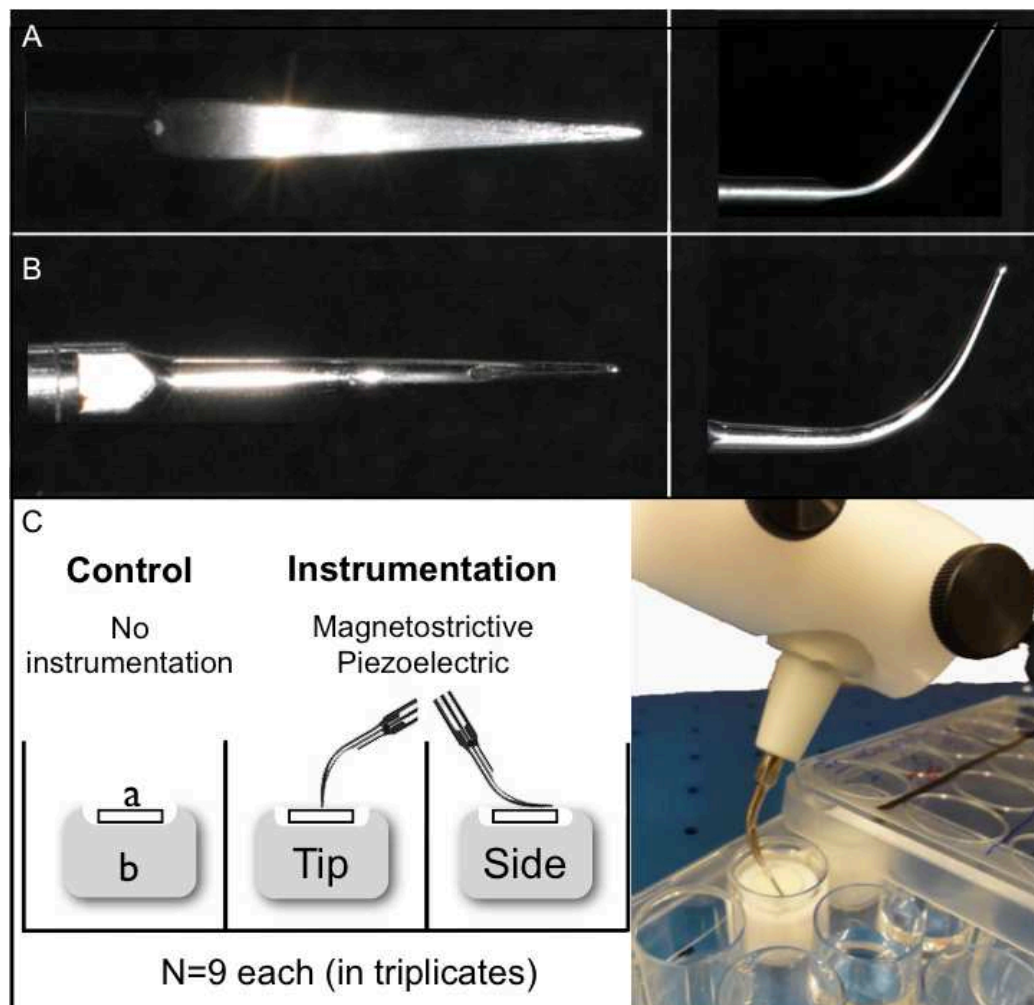


Fig. 2

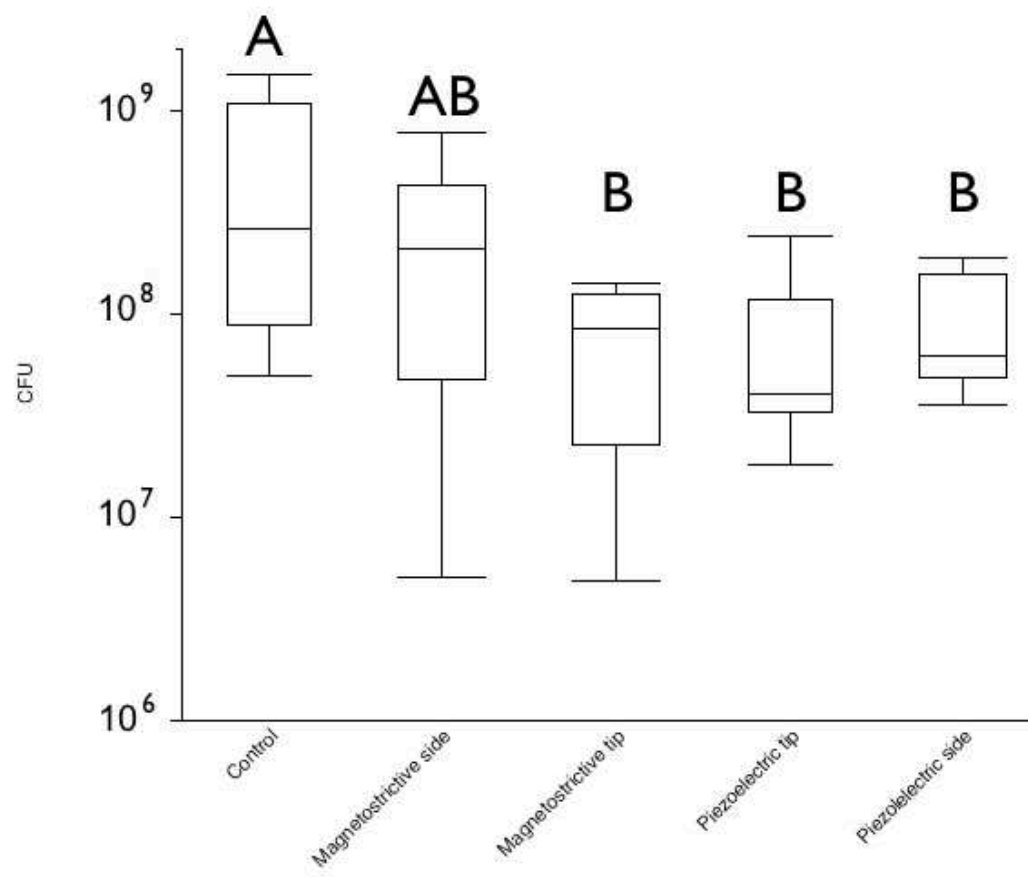


Fig. 3

